



Maxx Laboratories  
chase@maxxlaboratories.com


SAMPLE NAME: Bacteriostatic Water  
SAMPLE CODE: QNJP-N3YJ  
RECEIVED DATE: 07/13/2026  
PUBLISHED DATE: 07/26/2026



|                   |                      |
|-------------------|----------------------|
| DECLARED IDENTITY | Bacteriostatic Water |
| MATRIX TYPE:      | BACTERIOSTATIC WATER |
| SAMPLE NAME:      | Bacteriostatic Water |
| SAMPLE SIZE:      | 10 mL                |
| LOT CODE:         | ARC-BW-037           |

| Sample                      | Test        | Specification        | Result       | Status   |
|-----------------------------|-------------|----------------------|--------------|----------|
| Benzyl Alcohol Assay (HPLC) | HPLC        | 0.9% (v/v) $\pm$ 20% | 0.92 % (v/v) | CONFORMS |
| Fill volume / Net content   | Gravimetric | —                    | 9.83 mL      | MEASURED |
| pH Determination            | pH          | 4.5 – 7.0            | 7.00         | CONFORMS |

## HPLC Chromatogram Report

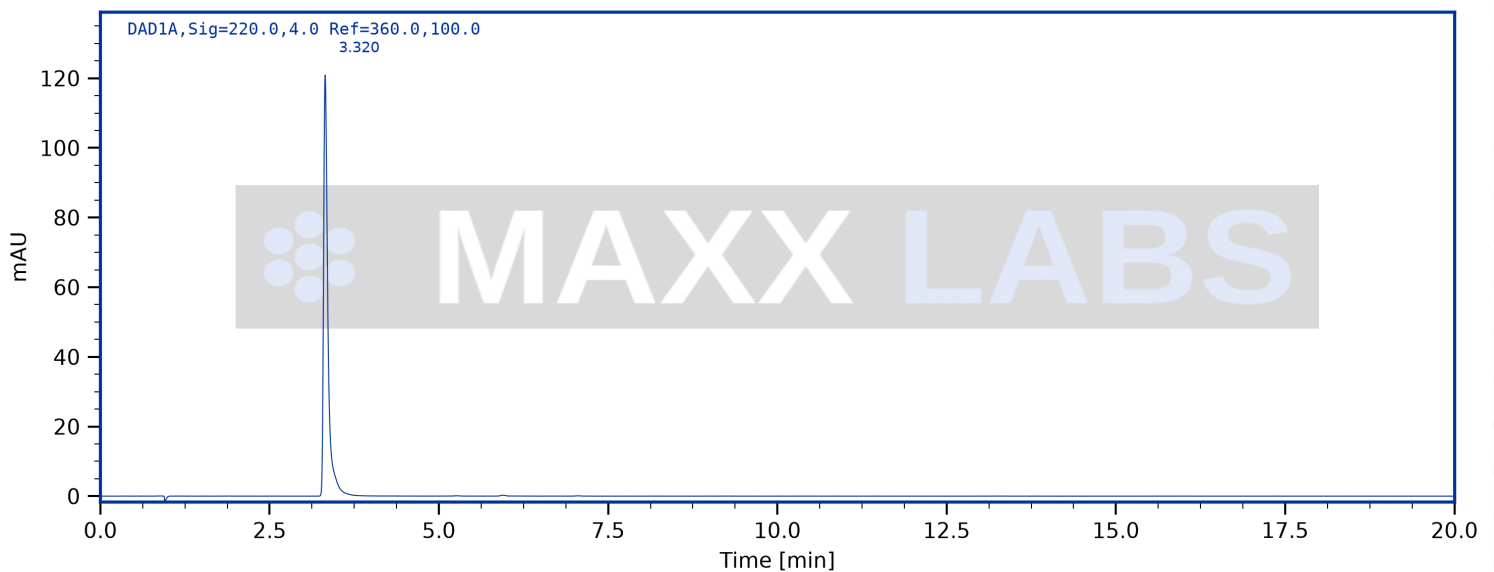

RESULTS REVIEWED BY:

Anthony Burke PhD  
Lab Manager  
07/26/2026

RESULTS CERTIFIED BY:

Dr. Levi Fried MD  
Lab Director  
07/26/2026

ACCUMARKLABS.COM  
QNJP-N3YJ  
07/26/2026





Maxx Laboratories  
chase@maxxlaboratories.com

SAMPLE NAME: Bacteriostatic Water  
SAMPLE CODE: QNJP-N3YJ  
RECEIVED DATE: 07/13/2026  
PUBLISHED DATE: 07/26/2026

| Sample               | Test                            | Specification     | Result | Status   |
|----------------------|---------------------------------|-------------------|--------|----------|
| Bacteriostatic Water | Endotoxin (LAL)                 | $\leq 0.25$ EU/mL | Pass   | CONFORMS |
| Bacteriostatic Water | Rapid Sterility Screening (PCR) | Not Detected      | Pass   | CONFORMS |

RESULTS CERTIFIED BY:

  
Anthony Burke PhD  
Lab Manager  
07/26/2026

RESULTS CERTIFIED BY:

  
Dr. Levi Fried MD  
Lab Director  
07/26/2026

ACCUMARKLABS.COM  
QNJP-N3YJ  
07/26/2026

